

Hospital **Vicenza ULSS 6 Vicenza**City **Vicenza**Country **Italia**

Rev	Date	Draftsman		Remarks
		Init	Signed	
A	08.12.1997	B.V.		NEW DRAWING
B	08.08.2000	E.K.		Repl. oxy and hardsh. by affinity, added 14-15-16
C	11.09.2003	R.R.		Several changes
D	10.10.2003	R.R.		Removed In 1,2,3,5,7 and added In 24,25,26,27
E	08.12.2005	J.U.		Changed line 22 & 24, added pressure
F	29.01.2007	E.K.		Duplicated line 9
G	05.04.2007	J.U.		Change line 15, add another line 9
H	06.12.2007	E.K.		Chg. 24-25-26-27-22-28-29, repl. 4 by 4a-4b
I	12.12.2008	J.U.		Not in use
J	12.12.2008	J.U.		Chg. 8, 14, 22, 26, remove 4a & 4b
K	22.12.2008	E.D.		Chg. lines 22 and 24
L	03.07.2009	C.V.		Turned oxygenator 180 degrees
M	11.09.2012	C.S.		Chg. to Fusion
N	08.11.2013	C.V.		Chg. table pack, line 22, item 28, 29
O	17.01.2014	C.V.		Not in use
P	17.01.2014	C.V.		Chg. 22, 24

PACKAGING INFORMATION CLEANROOM

Tray : Maxpack 1.00
 Lid : Tyvek Cover 1.00
 Bag :
 Label : End-label 1.00

NR

PACKAGING INFO PACKAGING DEPARTMENT

NR


U-Box : Maxpack box 1.00
 M-Box : **1 SETS IN 1 BOX**
 Inserts : MPbox insert 1.00
 Label : End-label 1.00
 IFU Custompack 1.00

Maxpack Tray







**DRAWING IS ACCORDING PROC. PE 2004
 REF. TO ALL APPLICABLE CLEANROOM PROC.
 AND Q.A. REQUIREMENTS
 ALL PACKS STERILIZED PER CYCLE 79**

Sterilisation load : 0.171 m³

APPROVAL	SIGNED	DATE
ENGINEERING		
MANUFACTURING		
QUALITY ASSURANCE		

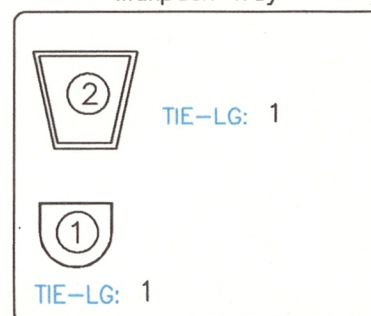

- ① FUSION OXY
 ② FUSION CVR ROTATED

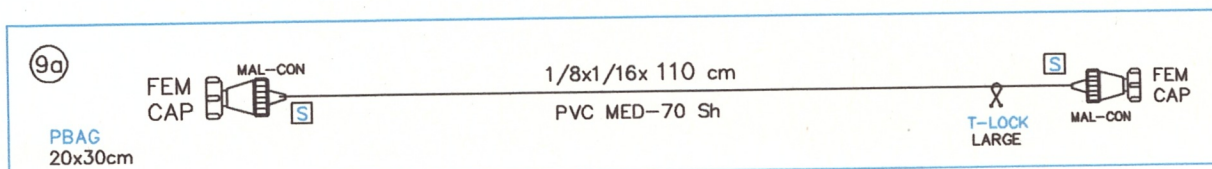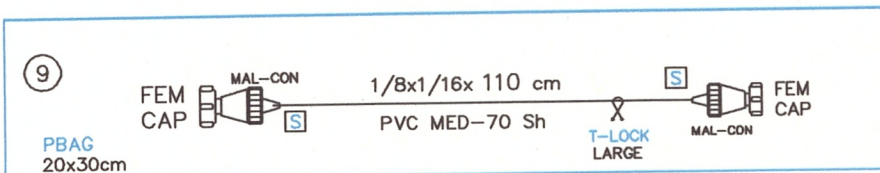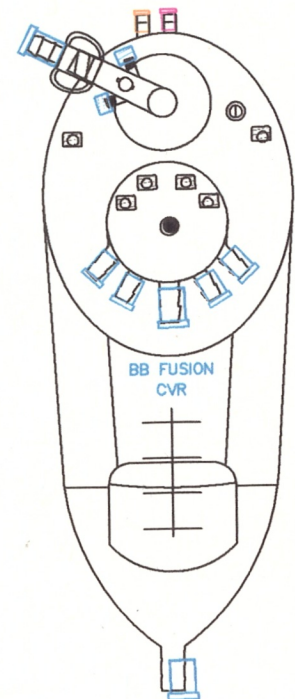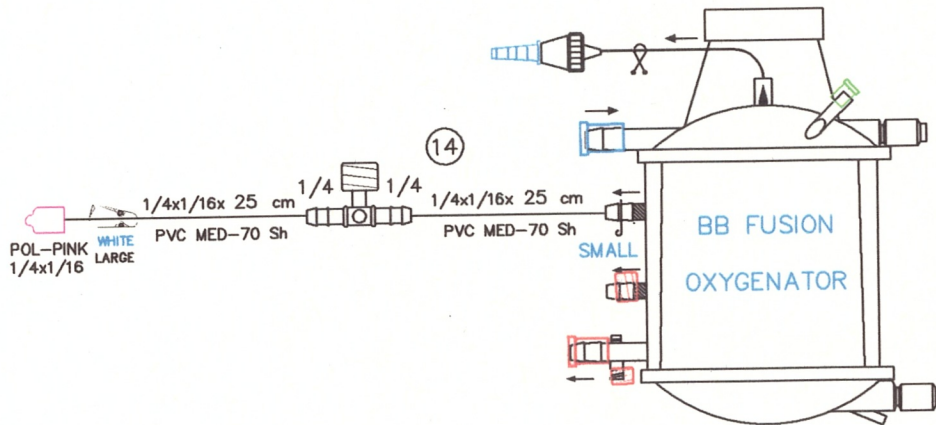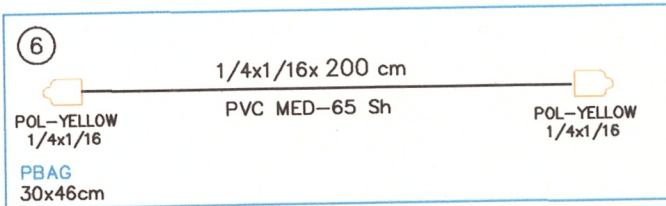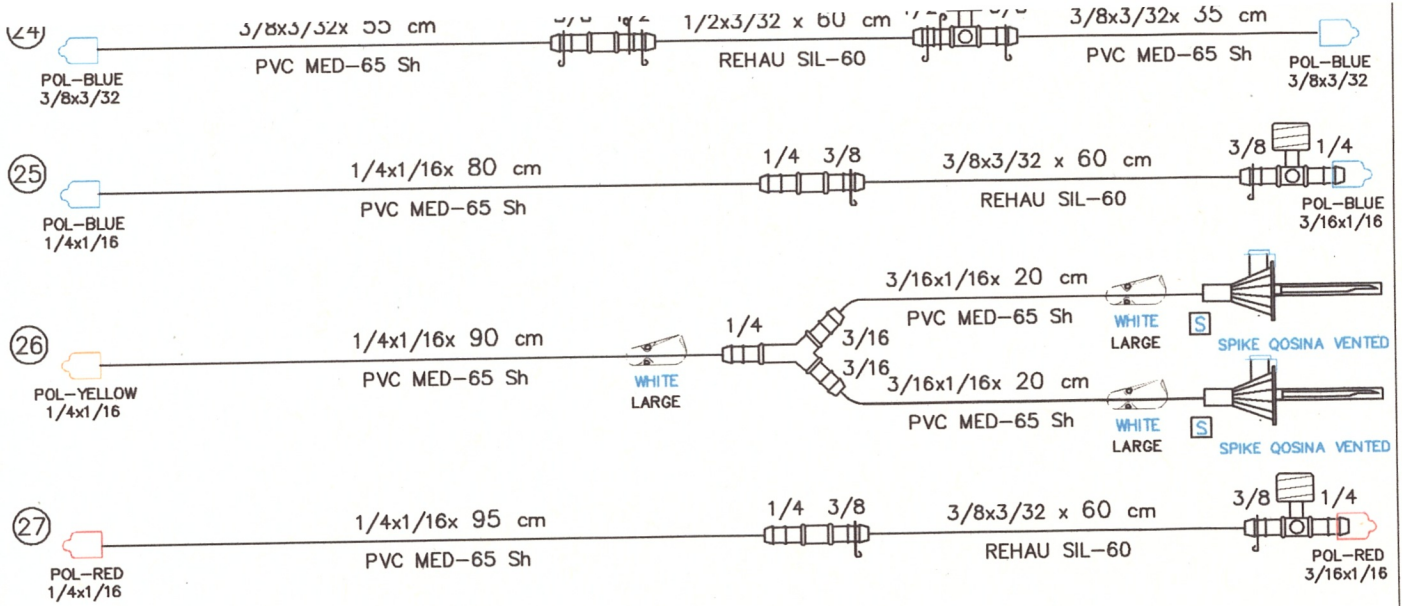



Button 1



TUBING HOLDER

180x80 mm
1/4

1/4  1/2

LEFT BLIND FOAM BLOCK

RIGHT FOAM BLOCK

Diagram illustrating a shield with five colored circles (black, red, blue) and labels W10, R12, B11, R13a, B13b.

TABLE TRAY + COVER

PBAG
50x90cm

Label: PACCO TAVOLO

